



Standard Config A

Cytometer:	LSRFortessa	User:	SaraPettersson
Cytometer Name:	LSRFortessa	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	12/3/2015 2:24:34 PM
Window Extension:	10.00		


Violet Laser
(405nm)

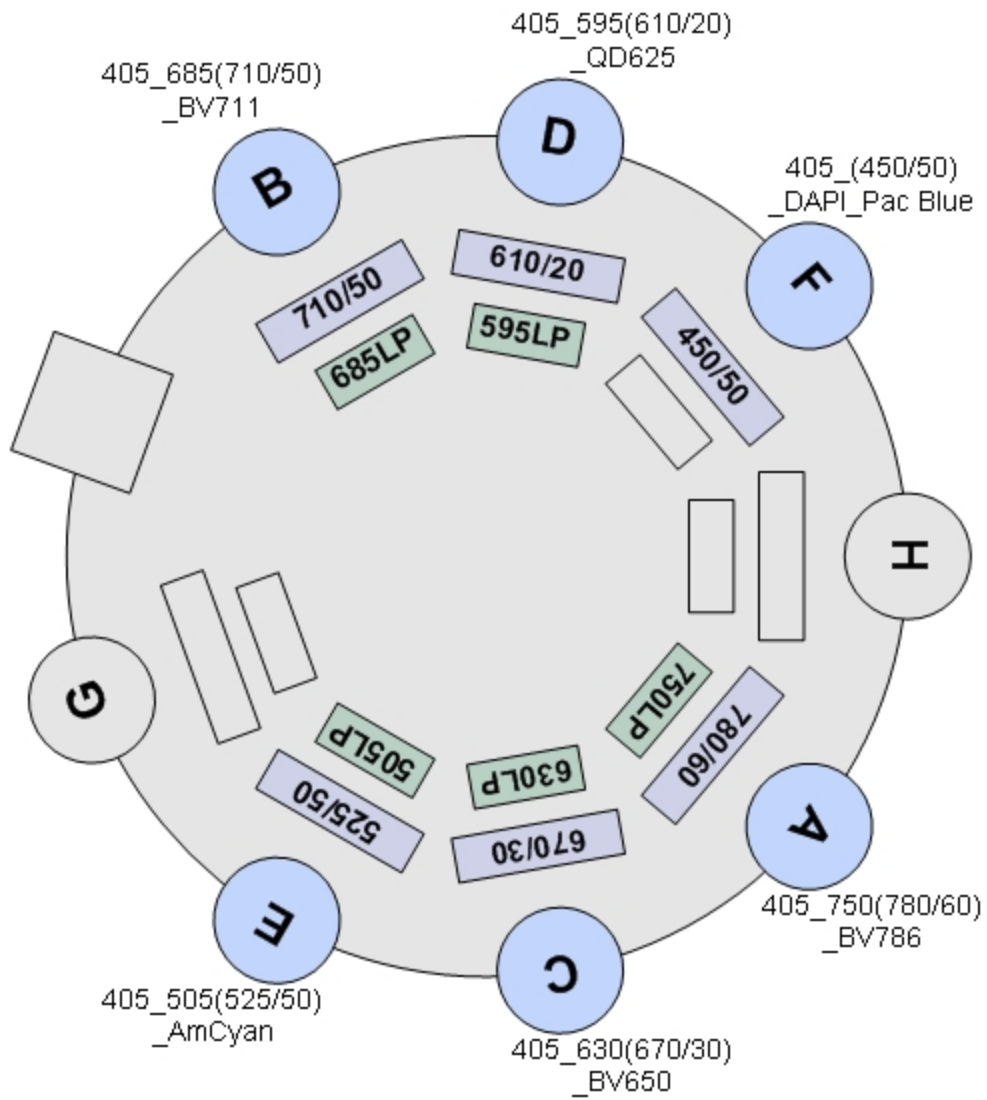


Red Laser
(640nm)

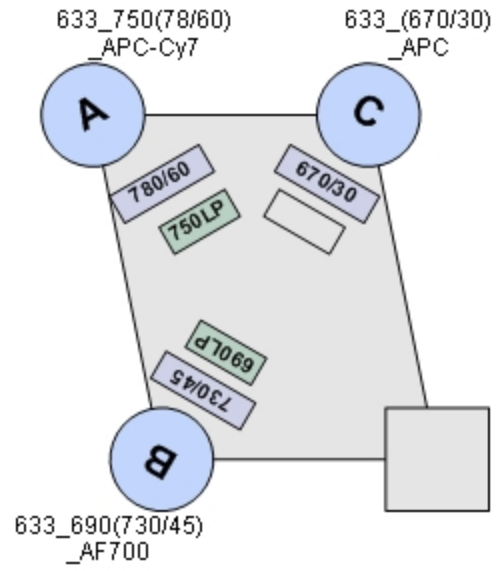


Yel Gr Laser
(561nm)

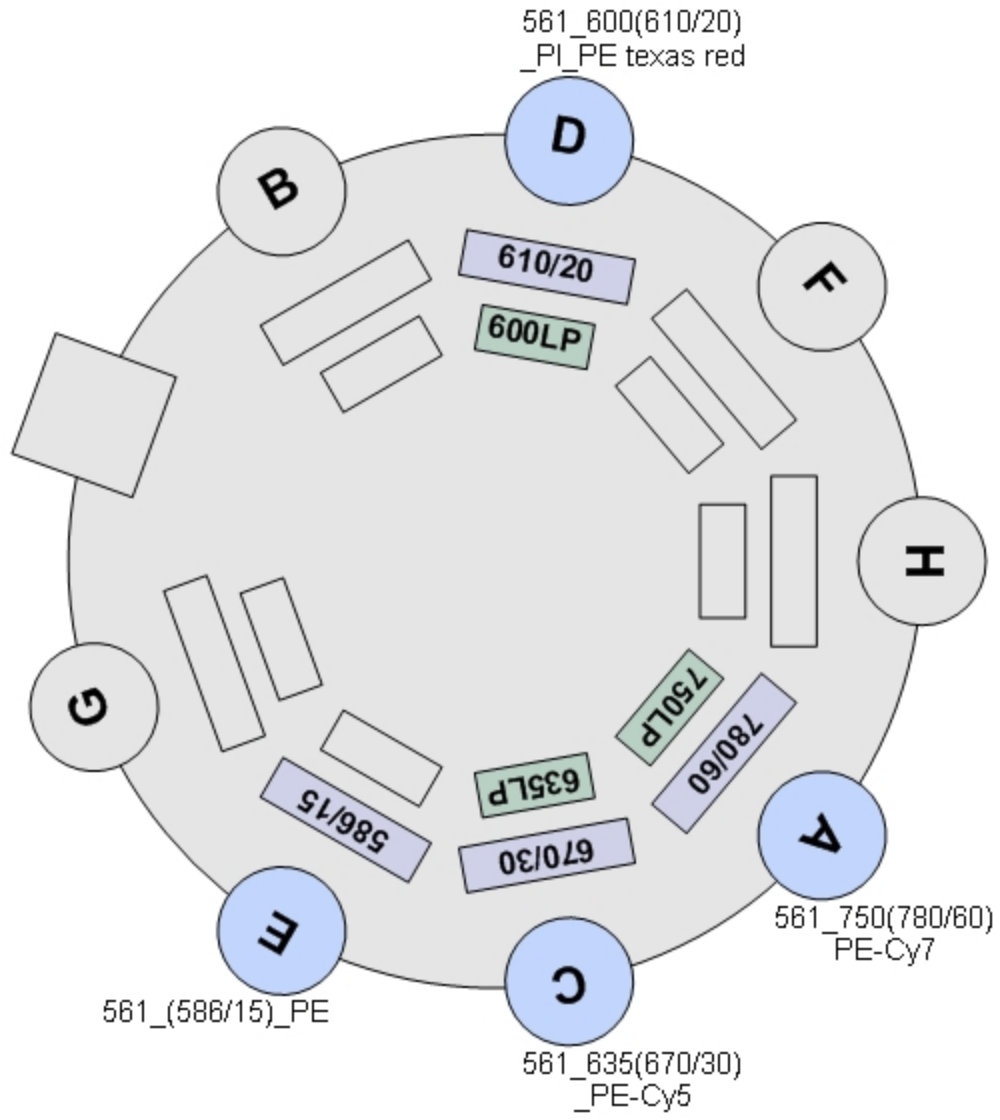

Blue Laser
(488nm)
FSC

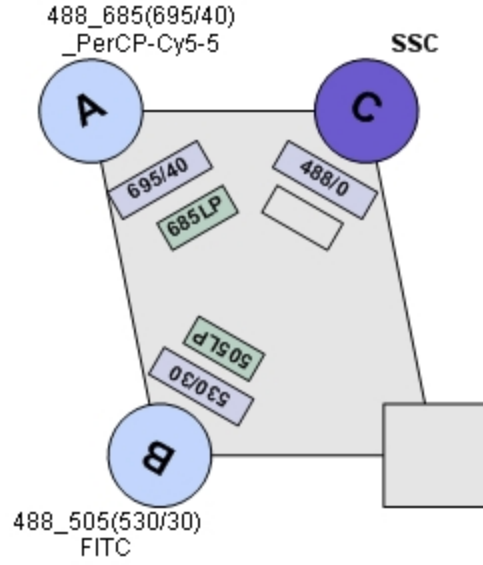

UV Laser
(355nm)

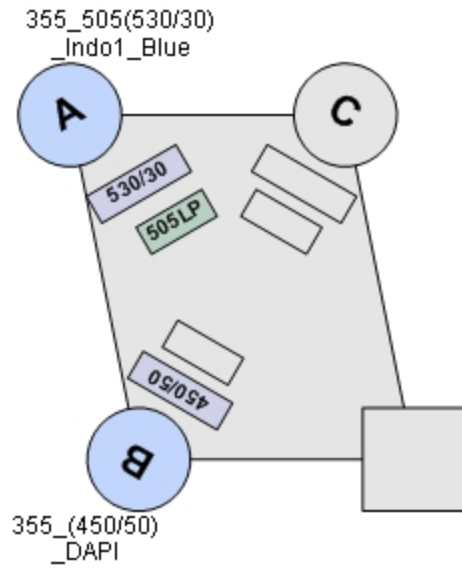

Comments: