



85 um (141125)SP

Cytometer:	FACSriaIII	User:	BioVis
Cytometer Name:	FACSriaIII	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	8/6/2015 2:59:12 PM
Sheath Pressure:	45.00		
Nozzle Size:	85		
Window Extension:	2.00		


Blue Laser
(488nm)
FSC

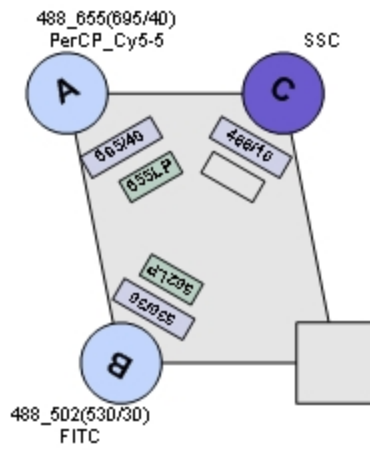


561 Yellow-Green Laser
(561nm)

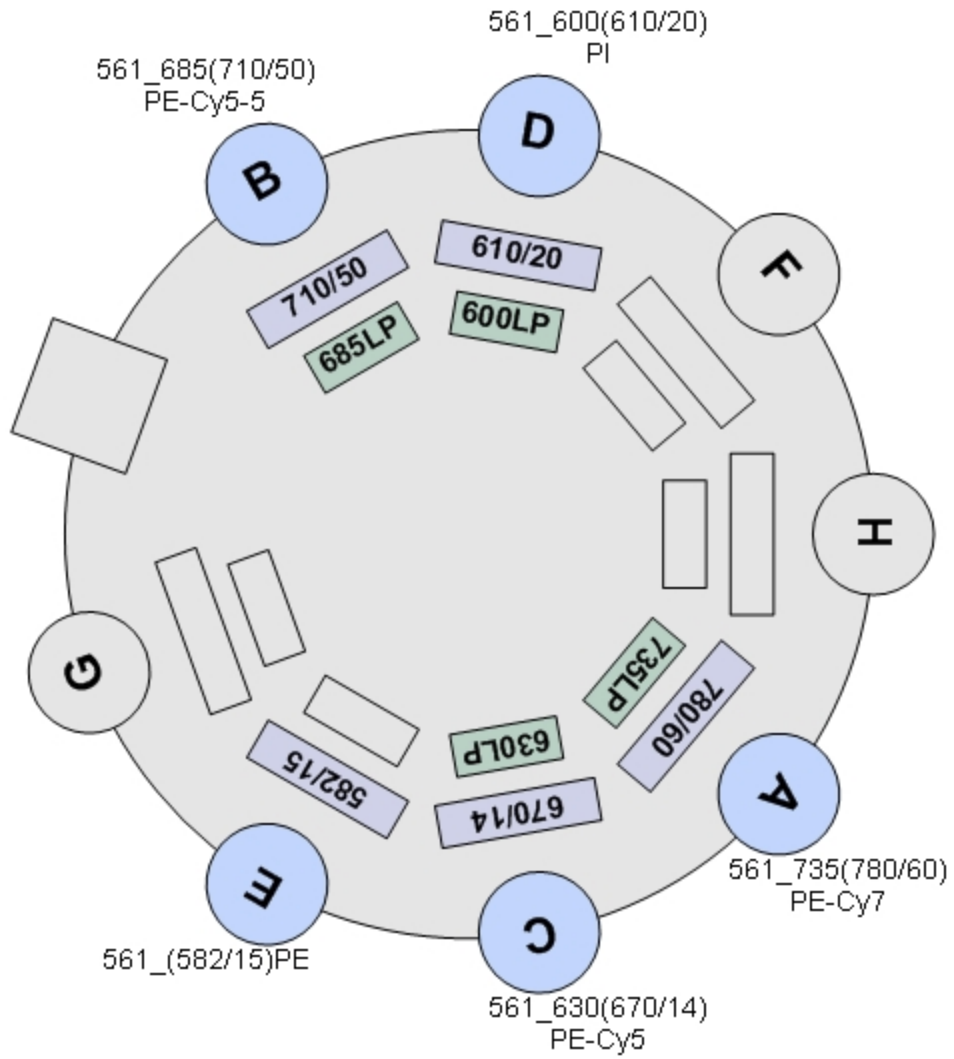

Red Laser
(633nm)

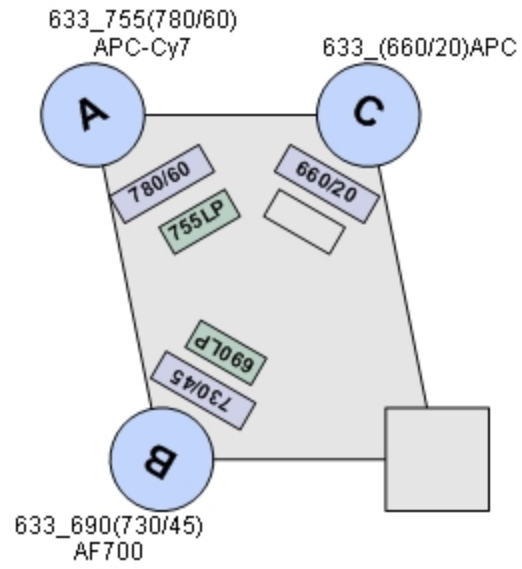

Violet Laser

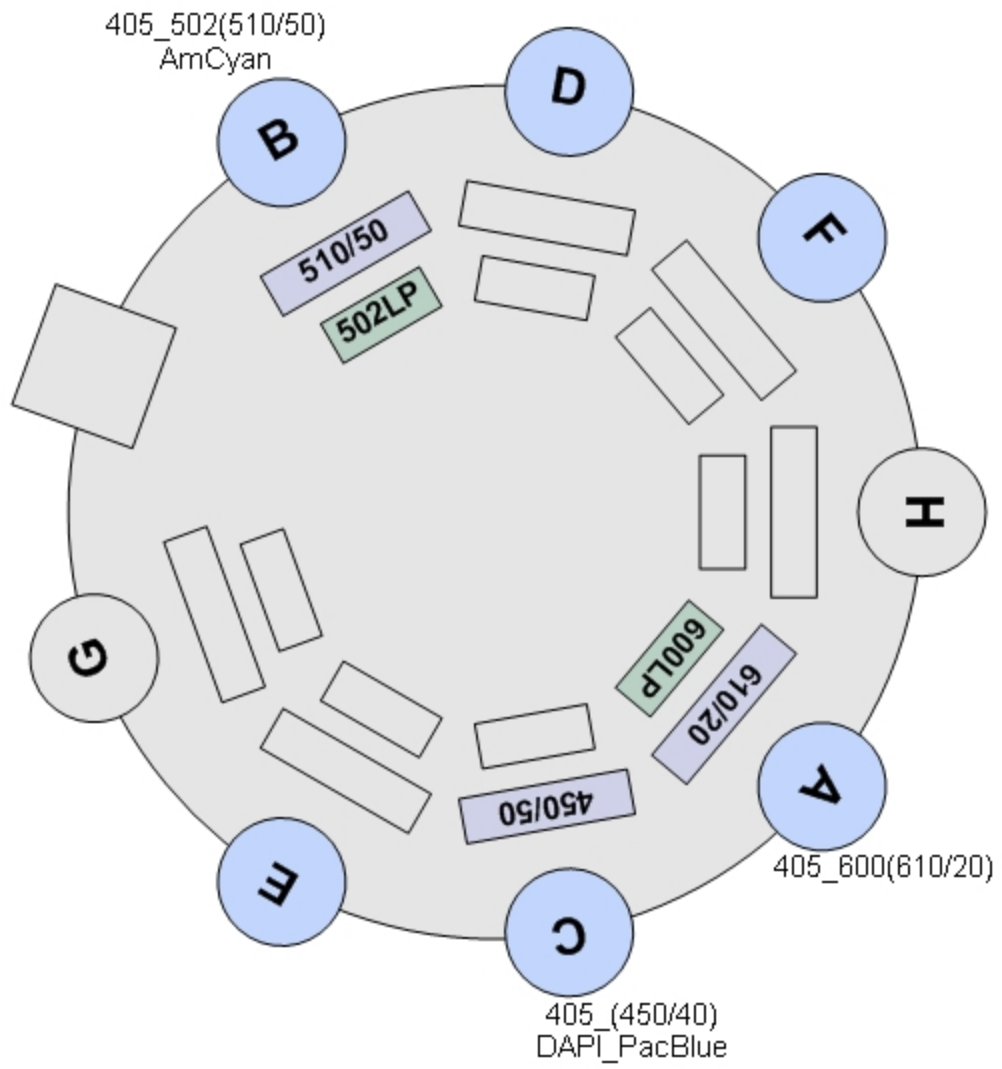

Comments: